





MANI TROCAR KIT

Ultimate Sharpness, Minimal Stress

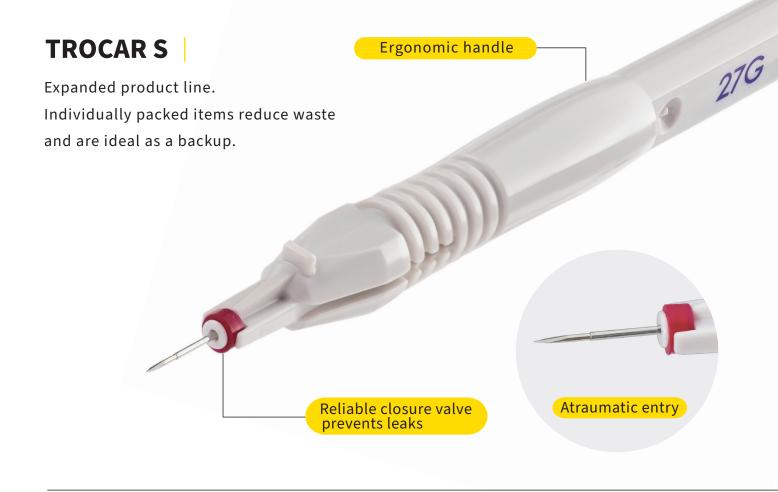

INFUSION CANNULA S



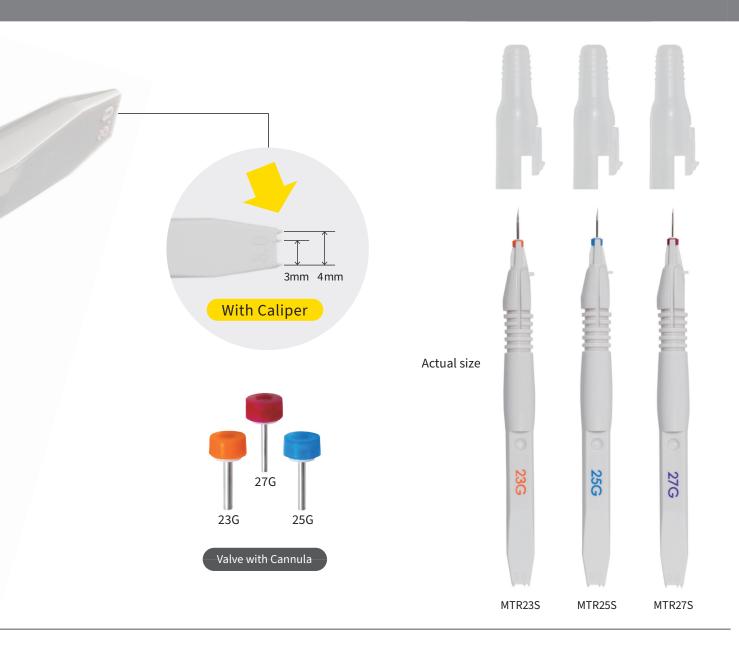

TROCAR KIT S



1 Surgery Case (1 Pack)

- TROCAR S × 3 Pcs.
- INFUSION CANNULA S × 1 Pc.
- * Individually packaged trocars are available for use as a fourth port or as a backup.



When holding the cannula

This product can be inserted into the sclera without holding the valved cannula. Withdraw the trocar handle after scleral placement. If the valved cannula does not detach easily, withdraw the trocar handle while gently holding the cannula with fine forceps. Take care not to touch the stop at the end of the handle as shown in the figure at right then position the cannula.

MANI TROCAR KIT

TROCAR KIT S

3 Kits/ Box

Description	Color Coding	Order No.
TROCAR KIT 27G S		MTK27S
TROCAR KIT 25G S		MTK25S
TROCAR KIT 23G S		MTK23S

TROCAR S

6 Pcs./ Box

Description	Color Coding	Order No.
TROCAR 27G S		MTR27S
TROCAR 25G S		MTR25S
TROCAR 23G S		MTR23S

^{*} Individually packed – ideal for backup

INFUSION CANNULAS

6 Pcs./ Box

Description	Color Coding	Order No.
INFUSION CANNULA 27G S		MIC27S
INFUSION CANNULA 25G S		MIC25S
INFUSION CANNULA 23G S		MIC23S

^{*} Individually packed – ideal for backup

C E 0197



